


Parts Introduction



1. Touchscreen
2. USB jack
3. Accessories frame
4. Channel 1
5. Channel 2
6. Channel 3
7. Channel 4
8. General power switch
9. Dust filter
10. Power supply line jack

Accessories

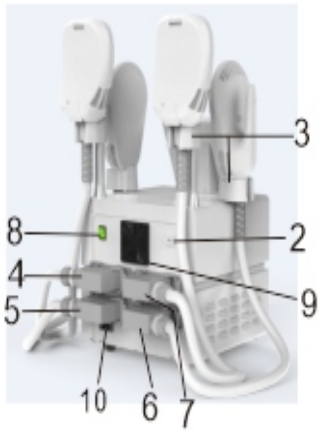

Accessories frame



work handle

Any part of instrument made of PMMA material (for example: accessories shelf, panel, transparent handles, etc.). Do not use alcohol or corrosive solvent to wipe clean.

Basal Operation

1.Put the accessories away and connect them to the mainframe.

(1)Insert the Channel 1 [4] jack;


(2)Insert the Channel 2 [5] jack;

(3)Insert the Channel 3 [6] jack;


(4)Insert the Channel 4 [7] jack;

2.Insert the plug of Power supply line into [10] socket, turn on Power switch [8]. the recharge interface enters the interface as (Fig 1) shows.

3.In the interface as (Fig 1):



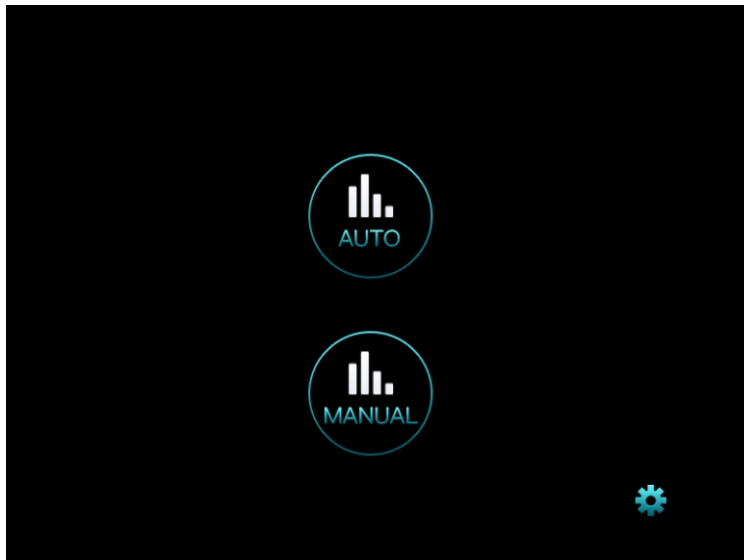

(1)Click on “” to select language. **Attention: The “Advanced setting” is only for manufacturer, Users do not use.**


(2)Click on “” to enter operating interface.




(Fig 1)

Auto Operation

- Clean treatment parts.
- In (Fig 1), click “AUTO” to enter (Fig 3) Select item according to the different gender, age and area (Select high medium and low according to different parts)energy of the guests than press “”to. Enter the operation interface of (Fig 4).
- Set work time. The system default work time is 30 minutes. Click on “+” and “-” of “Time setting” to regulate. The range is 1 to 30 minutes. Each part about 15 to 20 minutes.
- Set intensity. “AB” is the output strength of left and right handles by default. According to the bearing capacity of the guests Click on “+” and “-” of “Intensity” to adjust. The range is 1% (weak) to 100% (strong). When the intensity is set to 0, the output strength is turned off.
- Click on “”, the system start work. If you need to pause, Click on “”.
- Put on a bandage for user. and put in the handpiece in. The output intensity should be regulated from low gradually to high energy according to endurance of customers. During operating. The beautician should communicate with customers in time and the customers should tell how they feel .
- The system will pause automatically if the setting time is over.
- Please turn off the general power switch and unplug the power supply line. other parts of the handle shall not be cleaned with alcohol or other organic solvents to avoid damage to the.
- Click on “” to return to (Fig 1).

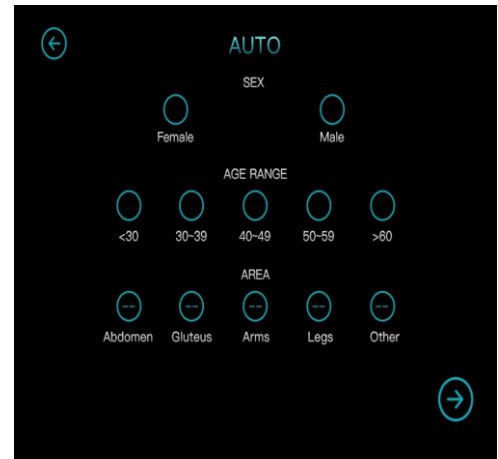


(Fig 3)

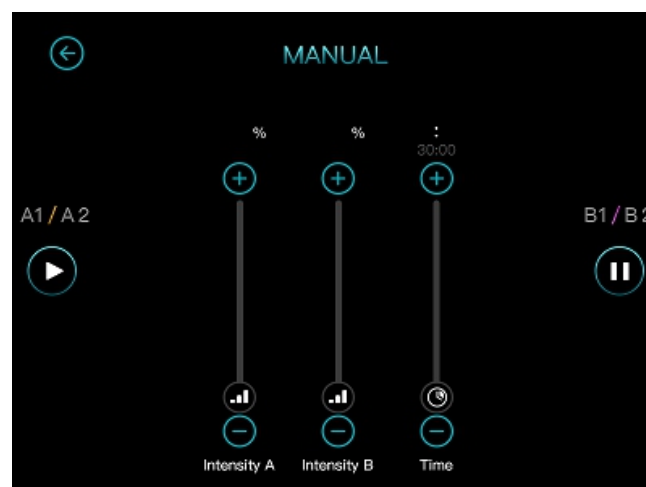

(Fig 4)

Manual Operation

1. Clean treatment parts.
2. In (Fig 1), click “MANUAL” to enter the interface (Fig 5). according to the different gender. It is suitable for fat rich parts.
3. Set work time. The system default work time is 30 minutes. Click on “+” and “-” of “Time setting” to regulate. The range is 1 to 30 minutes. Each part about 15 to 20 minutes.
4. Set intensity. “AB” is the output strength of left and right handles by default. According to the bearing capacity of the guests Click on “+” and “-” of “Intensity” to adjust. The range is 1%(weak) to 100%(strong). When the intensity is set to 0, the output strength is turned off.
5. Set frequency F1-F3. Click on “+” and “-” to adjust output Frequency System output strength starts to work. font turns green. font does not change. system output strength stops working. The range is: The range is 1HZ(slow) to 120HZ(Fast).
6. Set the storage mode. Select different modes and intensity according to the bearing capacity of the guests and Click on “▶” store. convenient Next use and query.
7. Click on “▶”, the system start work. If you need to pause, Click on “⏸”. the system start work.
8. Put a bandage for user. and put in the handpiece in. The output intensity should be regulated from low gradually to high energy according to endurance of customers. During operating. The beautician should communicate with customers in time and the customers should tell how they feel .
9. The system will pause automatically if the setting time is over.
10. Please turn off the general power switch and unplug the power supply line. other parts of the handle shall not be cleaned with alcohol or other organic solvents to avoid damage to the.
11. Click on “◀” to return to (Fig 1).

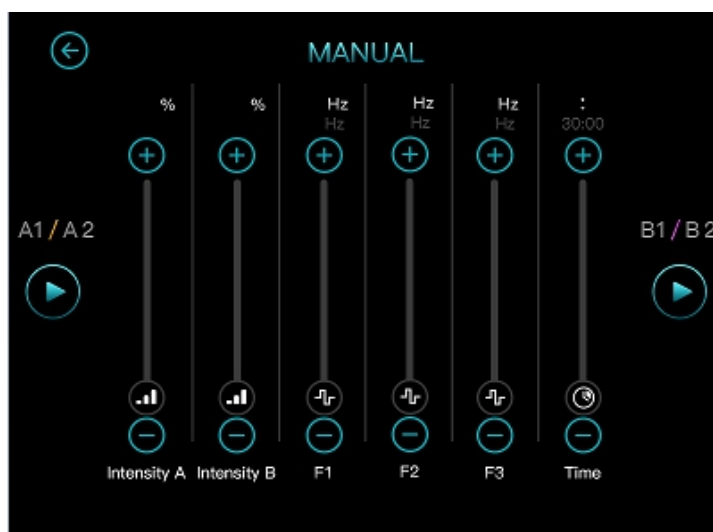

(Fig 5)

Forbidden Group



1. People with heart disease or high blood pressure, or configured cardiac pacemaker.
2. Patients with acute inflammation, asthma, deep vein thrombosis, thyroncus, cancer.
3. People with hemorrhagic disease, trauma or who is bleeding.
4. Pregnant women and child.
5. Medical Plastic parts, or parts with artificial in filling inside.
6. People with metal inside the body.
7. Patient with skin inflammation or with edema.
8. People with an abnormal immune system.
9. Numb or insensitive to heat.

Technical Parameters


Input Voltage: AC100~240V 50/60Hz □

Output Power: ≤1500VA






Fuse: RT28-32(RO15)20A 500V (with spare fuse)

Packing List

1.Host	1SET	<input type="checkbox"/>
2.Handle	4PCS	<input type="checkbox"/>
3.Power supply line	1PCS	<input type="checkbox"/>
4.User manual	1COPY	<input type="checkbox"/>
5.Accessory frame	4PCS	<input type="checkbox"/>
6.Binding(0.75M)	2PCS	<input type="checkbox"/>
7.Binding(1.5M)	1PCS	<input type="checkbox"/>
8.Binding(0.8M)	2PCS	<input type="checkbox"/>
9.Hexagnal screw wrench	1PCS	<input type="checkbox"/>
10.screw(4*8)	4PCS	<input type="checkbox"/>



Symbols and Meanings

Warning Symbol	Meaning
 Danger	If used incorrectly will bring the risk of death or serious injury!
 Warning	If used incorrectly will cause possibility ill of death or serious injury!
 Attention	If used incorrectly will cause personnel injury or damage to the goods!
 Danger	Device exists high pressure risk of high voltage output terminals!
 Warning	If used incorrectly will cause personnel injury!

*Things damage refers to housing, property, livestock and pet damage.

Contraindications

1. The following symptoms were forbidden to use

- (1) Patients who used by Heart rate regulator, cardiac pacemaker, ECS;
- (2) The use of artificial bone; Patients with silicosis;
- (3) Drunk or high fever patients;
- (4) Patients with higher sensitivity mental disease and epilepsy patients
- (5) Patients with no independent expression consciousness and can not take care of themselves.
- (6) Patients with metal materials in body (including metal teeth), pregnant women, cachexia, malignant tumor.
- (7) Severe hypertension and severe patients with cardiovascular and cerebrovascular disease.
- (8) Patients with renal failure.
- (9) Patients with severe infection



2. The following please use under the guidance of professionals

- (1) Women during menstruation;
- (2) Children;
- (3) Hemorrhagic disease or trauma, inflammation, skin disease, skin infection;
- (4) Patients with feeling numb, no response to cold and heat;
- (5) The immune system has defects, scar formation history, physical disease;
- (6) The people who has taken face-lifting or her body has artificial thing.




Maintenance

1. Appliances and medical equipment close to the machine may be resulting in operational failure due to interference.
2. Prohibit use of the equipment in the following environment
 - Hot and humid environment ——Dusty environment
 - Environmental with much smoke or steam
3. If there comes a failure, please shut down the power immediately, and send it to the distributor or manufacturer for maintenance. Do not repair by yourself.

4. Exclusion of liability.

The Company is not responsible for the following circumstances:

- (1) If fire, earthquake, war occurred;
- (2) The fault of the user, operator error;
- (3) Damage caused by using other method (not included in the use manual);
- (4) Operate without the manual's guide.

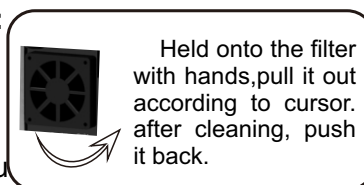

5. After using the machine for over 40 hours, please take off the dust filter and clean it (If have).
6. Do not make the machine close to the wall, keeping a 30CM space around for cooling.

Safety and Environmental Considerations

Toxic and hazardous substances reference list Electronic information product pollution control and management measures Table of contents of toxic and hazardous substances or elements

Part Name	Toxic and Hazardous Substance or Element						Remark
	Lead (Pb)	Mercury (Hg)	Cadmium (Cd)	Hexavalent chromium (Cr(VI))	Polybrominated biphenyls (PBB)	Polybrominated diphenyl ethers (PBDE)	
Plastic Board	○	○	○	○	○	○	
Printed Circuit Board	×	○	○	○	○	○	
Power Supply	×	○	○	○	○	○	
Accessory	×	○	○	○	○	○	

Declaration:

- The content of the restricted substances in all homogeneous materials of this part is below the limits set by the SJ/T11363-2006 standard.
 - ×
- The content of a homogeneous material in the part of the material is beyond the SJ/T11363-2006 standard requirements. The user's normal use of this product within the time limit of environmental protection, these substances or elements will not occur leakage or sudden change, will not cause the personal, property damage. For such substances or elements, the user shall not dispose of it yourself, please according to government regulations to the relevant departments of the government designated recycling.